


User Guide

EXTECH[®]
INSTRUMENTS
A FLIR COMPANY

ExStik™ Waterproof pH Meter

Model PH100

Patent Pending

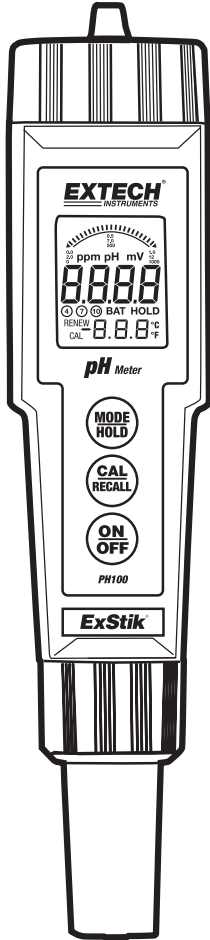


CE

ExStik™ Description

Front Panel Controls


1. Battery compartment cap
2. LCD Display
3. MODE / HOLD button
4. CAL / RECALL button
5. ON/OFF button
6. Electrode collar
7. Electrode

(Electrode cap is not shown)

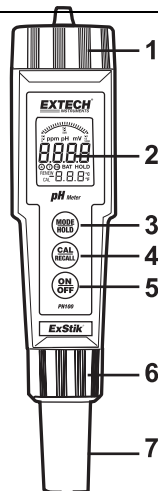

Display

1. Bargraph reading
2. Measurement reading
3. BAT (low battery) and HOLD (data hold) indicators
4. Temperature display
5. Bargraph scale designations
6. Units of measure
7. Calibration indicators
8. RENEW and CAL indicators

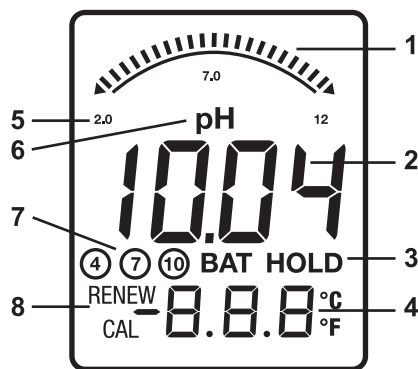

CAUTIONS

- This device is not a toy and must not reach children's hands. It contains hazardous objects as well as small parts that the children could swallow. In case a child swallows any of them, please contact a physician immediately
- Do not leave batteries and packing material lying around unattended; they can be dangerous for children if they use them as toys
- In case the device is going to be unused for an extended period of time, remove the batteries to prevent them from training
- Expired or damaged batteries can cause cauterization on contact with the skin. Always, therefore, use suitable hand gloves in such cases
- See that the batteries are not short-circuited. Do not throw batteries into the fire.

Overview

pH Overview

pH is a unit of measure (ranging from 0 to 14pH) indicating the degree of acidity or alkalinity of a solution. pH tests are the most commonly performed measurements in water analysis and reports the negative log of the hydrogen ion activity of a solution which is an indicator of acidity or alkalinity. Solutions with a pH less than 7 are considered acidic, solutions with a pH higher than 7 are known as bases, and solutions with a pH of exactly 7 are neutral.

The pH scale is logarithmic so, for example, if sample A is 1 pH less than Sample B, this means that Sample A is 10 times more acidic than Sample B. A difference of 1 pH represents a ten-fold difference in acidity.

Getting Started

- For new meters, remove the battery cap and then remove the battery insulating strip.
- Remove the cap from the bottom of the ExStik™ to expose the electrode glass surface and reference junction
- Before first use or after extended storage, soak the electrode (with its cap removed) in a pH 4 solution for about 10 minutes
- White KCL crystals may be present in the cap. These crystals will dissolve in the soak or they can be simply rinsed with tap water
- Always calibrate close to the expected measurement value
- Before a sponge is located in the electrode protective cap. Keep this sponge soaked with a pH 4 solution to preserve Electrode life during storage

Replacing Electrodes

The ExStik™ is shipped with an electrode attached. Electrode life is limited and is dependent on (among other factors) frequency of use and care. If the electrode needs to be replaced, follow these steps for removing and connecting electrodes.

1. To remove an electrode, unscrew and completely remove the electrode retaining collar.
2. Gently rock the electrode from side to side, pulling it away from the meter, until it disconnects.
3. To attach an electrode, carefully plug the electrode into the meter socket (note that the electrode connector is keyed, ensuring proper connection).
4. Secure the electrode in place by tightly turning the collar in place. (a rubber gasket seals the electrode with the meter).

Automatic Electrode Recognition

When the ExStik™ is turned on, it recognizes the type of electrode that is connected and displays the appropriate unit of measure. Attach electrode before turning the ExStik™ on.

Powering the ExStik™

Press the ON/OFF key to turn the ExStik™ on or off. The auto power off feature shuts the ExStik™ off automatically after 10 minutes of inactivity to preserve battery life.

Operation

Overview

When the electrode is placed in a solution, the main display and bargraph indicate the pH reading while the lower display reads temperature (readings flash until they have stabilized). The bargraph is 'center zero', i.e. at pH 7 there is no display. As the pH rises, the bar moves from the center to the right. If the pH drops, the bar moves from the center to the left.

pH Calibration (1, 2, or 3 points)

A two point calibration with a buffer of 7 plus 4 or 10 (whichever is nearest to the expected sample value) is always recommended. A one point calibration (choose the value closest to the expected sample value) is also valid. For best accuracy, always calibrate at the sample temperature.

1. Place the electrode into a buffer solution (4, 7, or 10) and momentarily press the CAL key. pH 7 should be calibrated first, then 4 and/or 10 pH.
2. The ExStik™ automatically recognizes the solution and calibrates itself to that value.
Note: If the solution is more than 1pH off from the 4, 7, or 10pH standard, the ExStik™ will assume an error and abort the calibration. CAL and END will be displayed.
3. During calibration, the pH reading flashes on the main display.
4. When calibration is complete, the ExStik™ automatically displays 'END' and returns to normal operation mode.
5. The appropriate circled indicator ④, ⑦, or ⑩ will appear on the LCD when a calibration has been completed. The calibration data is stored until a new calibration is performed.
6. For a two or three point calibration, repeat steps 1-4.

Note: Always turn the meter off and then on before calibrating to allow sufficient time to complete the calibrations during one power cycle. If the meter auto powers off during calibration the calibrations remain valid, but new calibrations will turn the circled indicators off.

Changing the Displayed Temperature Units


Press and hold the CAL button for approx. 3 seconds. The °C or °F icon will change first and the numerical temperature value will change *after* the button is released. If the Calibration mode is accidentally accessed 'CAL' appears on the LCD. Simply turn the ExStik™ off and start again.

Data Hold

Momentarily press the MODE button to freeze the current reading. The HOLD display icon will appear along with the held reading. The held reading will also be stored in memory. Momentarily press the MODE key to return to normal operation.

15-Storing Readings into Memory

1. Momentarily press the MODE button to store a reading. The LCD will briefly display the memory location number and then the value stored (Data Hold will activate).
2. Momentarily press MODE again to return to normal operation.
3. Repeat step 1 to store the next reading and so on.
4. After 15 readings are stored the ExStik™ will return to memory location 1 and start overwriting existing data with newly stored data.

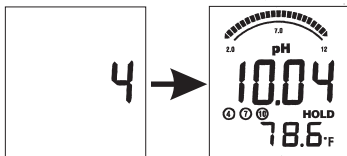

Recalling Stored Readings

Note: Check that the HOLD symbol is not displayed. If it is, exit the HOLD function by momentarily pressing the MODE button.

1. Momentarily press the CAL button and then press the MODE button immediately after CAL is displayed; the storage location number (1 through 15) will flash. If the CAL mode is accidentally accessed (display flashing), press the CAL button again to exit.
2. The last reading stored will be displayed first. To advance through the stored readings, momentarily press the MODE button. The location number is displayed first, followed by the reading stored in that location.
3. To exit the recall mode, momentarily press the CAL button and the ExStik™ will return to normal operation.

CAL Reminder Display

When the ExStik™ is turned on in the pH mode for the 15th time without recalibration, the 'CAL' icon appears on the LCD indicating that the ExStik™ may require calibration. Some applications may require recalibration of the electrode more frequently than others. The CAL display is simply a reminder and will turn off when the pH electrode is recalibrated.

RENEW Display


A flashing 'RENEW' warning indicates that the probe may be nearing the end of its useful life. If cleaning or recalibration does not cause the RENEW icon to disappear, replace the electrode. The RENEW display appears when the output of the pH electrode fails a diagnostic test.

Considerations

- If the unit appears to be locked (display frozen) it is possible that the Data Hold mode has been inadvertently accessed by pressing the MODE button. Simply press the MODE button again or turn the meter off and restart if the display appears frozen.
- If the meter does latch up and no button presses revive it, remove the batteries, push the ON button for 3 seconds and then reinsert the batteries.
- Note that if the batteries are removed, any stored readings will be discarded. Also, the user calibration data for pH will be cleared. New user pH calibration data is required. Factory calibration data for all models will be retained, however.

Battery Replacement

1. Twist off the battery compartment cap
2. Replace the four (4) 2032 batteries observing polarity.
3. Replace the battery compartment cap

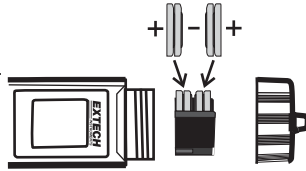

You, as the end user, are legally bound (**Battery ordinance**) to return all used batteries and accumulators; **disposal in the household garbage is prohibited!** You can hand over your used batteries / accumulators, gratuitously, at the collection points for our branches in your community or wherever batteries / accumulators are sold!



Disposal

Follow the valid legal stipulations in respect of the disposal of the device at the end of its lifecycle

Specifications

Display	Multifunction LCD with Bargraph
Operating conditions	0 to 50°C (32 to 122°F) / < 80% RH
Range and Accuracy	0.00 to 14.00 / ± 0.01pH typical
Temp. Compensation	Automatic from 0 to 90°C (32 to 194°F)
Temperature Range	-5 to 90°C (23 to 194°F)
Temperature Resolution	0.1° up to 99.9 then 1° thereafter
Temperature Accuracy	± 1°C/1.8°F [from -5 to 50°C (23 to 122°F)] ± 3°C/5.4°F [from 50 to 90°C (122 to 194°F)]
Measurement storage	15 tagged (numbered) readings
Power	Four (4) CR2032 button batteries
Low battery indication	'BAT' appears on the LCD
Auto power off	After 10 minutes of inactivity
Dimensions	35.6x172.7x40.6mm (1.4x6.8x1.6"); 110g (3.85oz)

Copyright © 2008 Extech Instruments Corporation.

All rights reserved including the right of reproduction in whole or in part in any form.
www.extech.com

airconcern

more info for Extech PH100

Phone: 01235 838 555

Email: cs@airconcern.co.uk

Web: www.airconcern.co.uk

Air Concern Ltd, Building 173 Curie Avenue Harvell Didcot, Oxfordshire